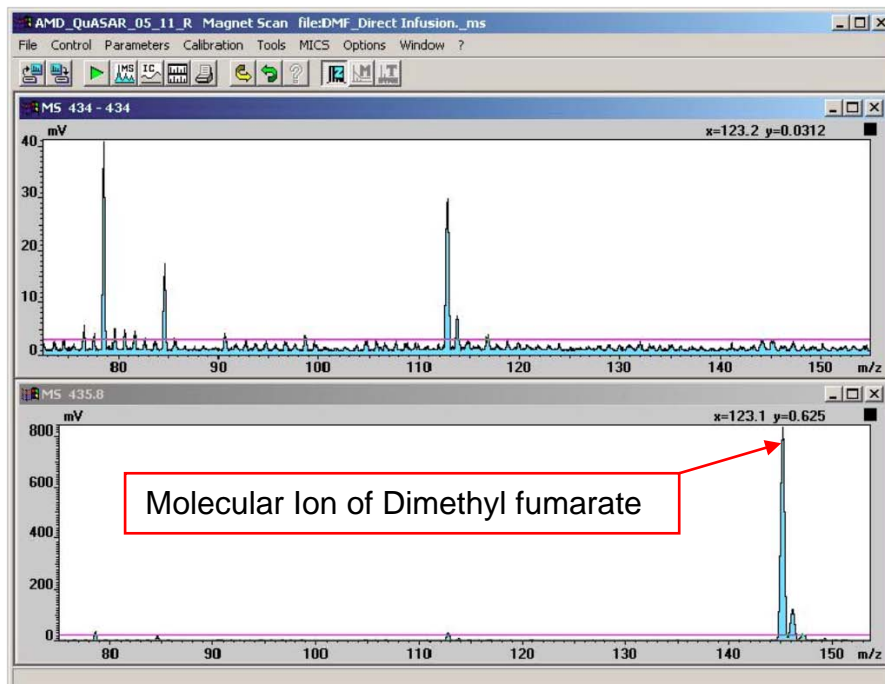
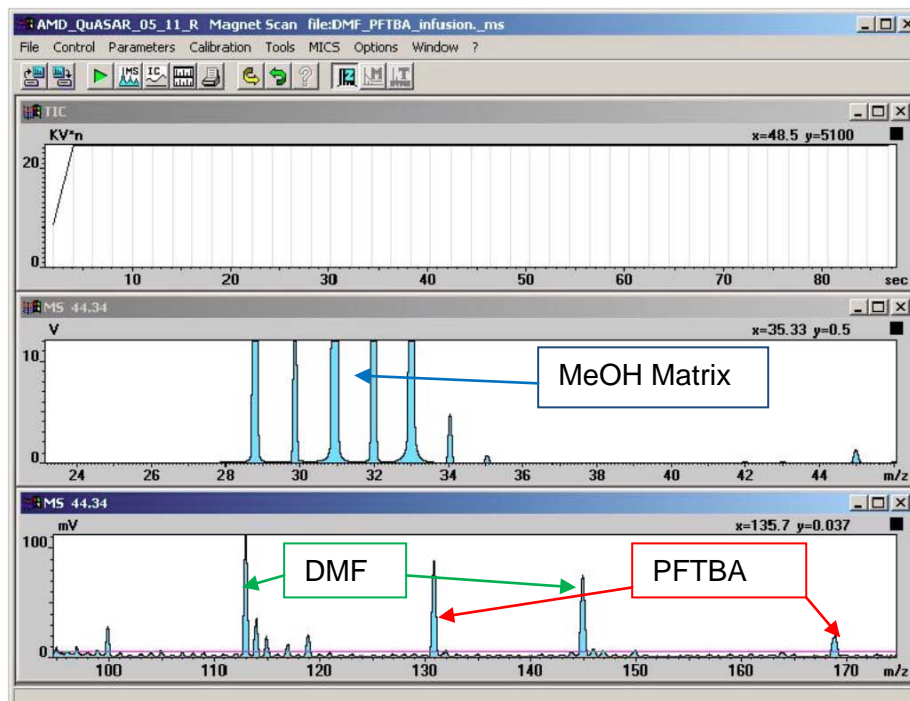


## Method Development



**Fig. 1** Direct Sample Infusion of 100ng/μl DMF at 1 μL/min solvent flow; EI mass spectrum



**Fig. 2** Direct Sample Infusion of DMF/PFTBA including solvent matrix at 1 μl/min; EI mass spectrum incl. Reference Compound for Mass Determinations

Rev. KHM/120711